UNIVERSITY
OF MIAMI

Rosenstiel School of Marine, Atmospheric, and Earth Science
Tritium Laboratory

4600 Rickenbacker Causeway
Miami, FL 33149-1031

P: 305-421-4100
F: 305-421-4112
tritium@miami.edu

Tritium Laboratory
21 October 2024

SWAB REPORT # 1104

SWAB DATE: 11 October 2024

University of British Columbia
Earth and Science Building

James Happell Digitally signed by James Happell Date: 2024.10.21 11:32:30 -04'00'

James D. Happell

Distribution:
SWAB Committee
Morgan Griffith

COMMENTS TO SWAB REPORTS 15 December 2021

The LSC is now a Quantulus GCT 6220, with the SWAB counting assay having background cpm of 0.3 & 1.2 for ^{3}H & ^{14}C. This replaces an LSC with background cpm of 1.6 & 5.5 for ^{3}H & ^{14}C.

All samples are counted for 60 minutes, the instrument background is subtracted, and activities are reported in dpm/m^2. Bucket blank activities are not subtracted. Counting errors (2 standard deviations) are also reported in dpm/m^2. An error larger than the activity indicates that the activity is not significantly different from zero. All activities significantly above background will be in **bold**.

Criteria for SWAB Results

Category	^{3}H (dpm/m^2)	^{14}C (dpm m^2)	Recommendations
A	<500	<50	No action
B*	500-10,000	50-10,000	Needs cleaning before any natural tracer work. Decks in radiation vans with activities above 1000 dpm/m^2 should be cleaned.
C**	10,000-100,000	10,000-50,000	Must be cleaned before any use.
D***	>100,000	>50,000	May be a health hazard. Notify local radiation safety official.

Note: ^{14}C and ^{35}S have peak energies of 156 and 167 KeV, respectively; thus ^{35}S will be registered as ^{14}C by our counting techniques. Categories A, B and C are not a health hazard.

Recommended Cleaning Proceedure

Wearing ordinary household rubber gloves:

^{3}H: Wash and scrub with radioactive cleanup detergent such as COUNT-OFF (50 ml COUNT-OFF to 4 liters of water), using sponges to distribute solution and reabsorb it.

^{14}C: Wash with 1% sulfuric or 2% hydrochloric (muriatic) acid with good ventilation (will dissolve carbonates, releasing $^{14}CO_2$). Follow up with wash as if for ^{3}H.

Disposal of Cleaning Materials (gloves, sponges, etc)

Categories A & B dispose as ordinary garbage, C & D contact your institution's radiation safety office.

Note: If category C or D is encountered, we try to notify the insitution promptly by phone or email.

REPORT FOR SWAB # 1104

LOCATION: Univ. of British Columbia DATE: 16 October 2024
VESSEL: Earth and Science Building TECHNICIAN: Morgan Griffith

Sample #	Sample Identification	^{3}H dpm/m^{2} activity	±	error	^{14}C dpm/m^{2} activity	±	error
1	1st Vial Bkgnd	0	±	0	0	±	0
2	Initial bucket blank	29	±	22	-7	±	20
3	Counter and floor in Groat lab where I w	5	±	21	3	±	15
4	Flow hood where I process samples for NO	**106**	±	**33**	-9	±	27
5	Floor in the aisle where I prepare sampl	**22**	±	**20**	4	±	12
6	Bench in the aisle where I prepare sampl	11	±	26	-8	±	24
7	Centrifuge	**23**	±	**8**	***122**	±	**20**
8	Floor in the aisle with RO water system	-5	±	21	-8	±	25
9	Floor in entryway of 3052	**49**	±	**26**	-9	±	26
10	Floor in fridge freezer room of 3052	**26**	±	**23**	-6	±	17
11	Benches in balance room and balances	**36**	±	**23**	-4	±	11
12	Freeze drier	**48**	±	**27**	-14	±	40
13	Dumbwaiter	**61**	±	**30**	-16	±	47
14	Hallway outside2062 rad room	0	±	5	1	±	14
15	Benches in aisle across from rad room	**31**	±	**24**	-9	±	27
16	Aisle with large flow hood and HPLC (flo	16	±	23	-4	±	15
17	Cabinets where glassware is stored and f	**41**	±	**24**	-4	±	16
18	Floors and counters in aisle with MQ sys	-2	±	9	-7	±	22
19	Entryway to 2062	-7	±	27	3	±	17
20	Small centrifuge	-1	±	5	-6	±	16
21	3042 Doorway into 3052	17	±	22	-5	±	14
22	3042 Main entrance	**30**	±	**26**	-12	±	36
23	3042 Center hallway	16	±	21	-2	±	28
24	3052 Glassware cabinet	-19	±	42	-7	±	19
25	Final bucket blank	12	±	13	10	±	14

Comments

Please note that the error reported for each isotope is the two-standard deviation counting error. Reports may now contain values less than zero. Decay counting background samples will be distributed about the background vial, which means that negative values are possible. In the past we rounded the negative values to zero. Values are only significantly above background when they are positive and larger than the error. Please note that we are now using a Quantulus 6220 LSC which counts very near natural background. While the cleanup standards have not changed all values above background will now be in bold. All areas were clean except fgor the centrifuge. This shooud be cleaned before processing background ^{14}C samples.

ESB 3052 FLOOR PLAN

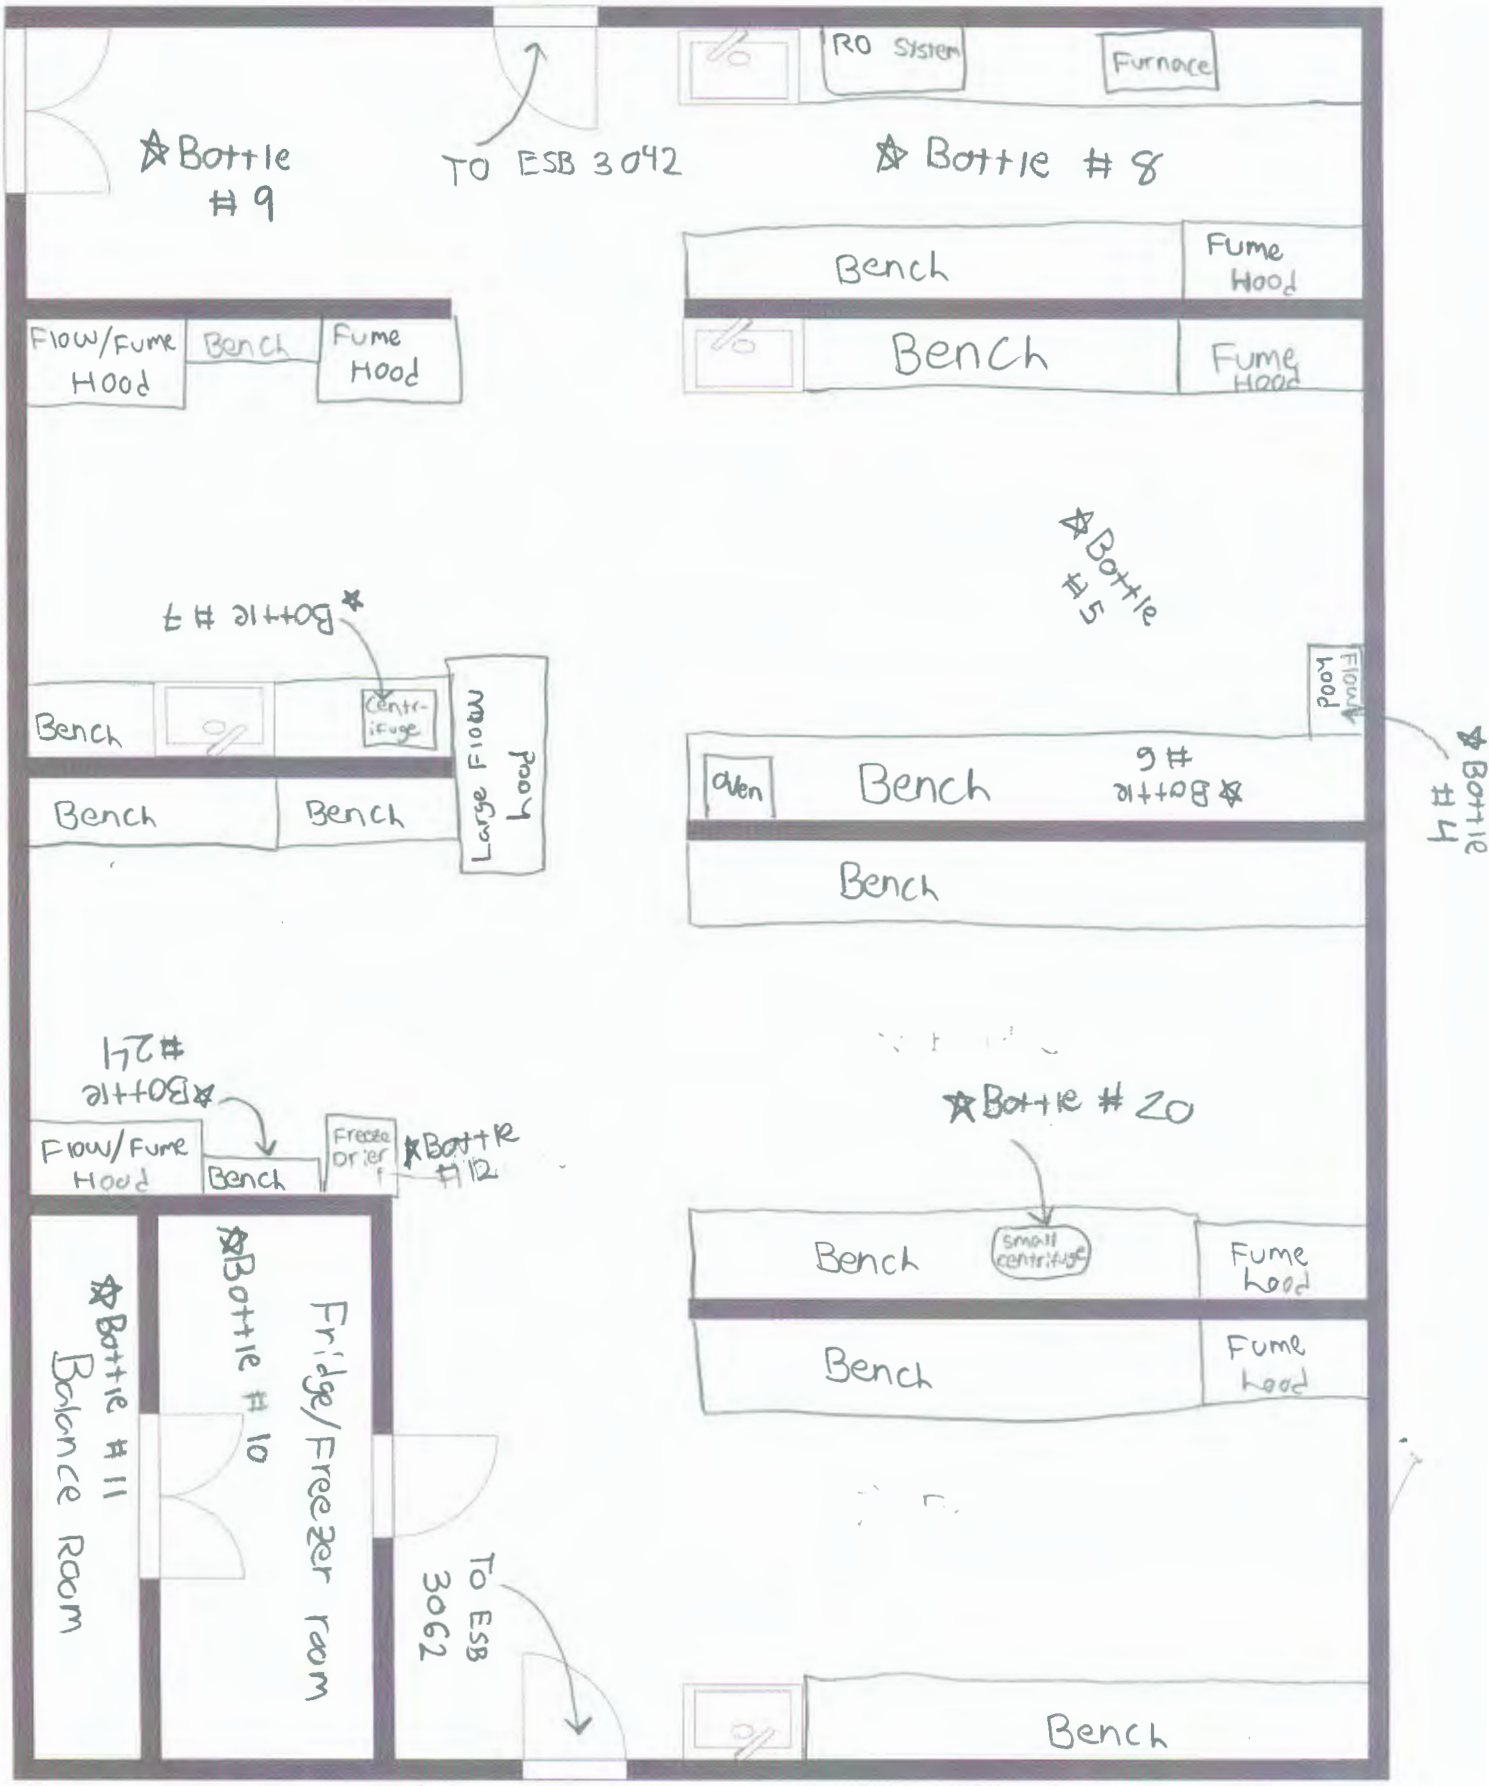

ESB 3042 Floor Plan

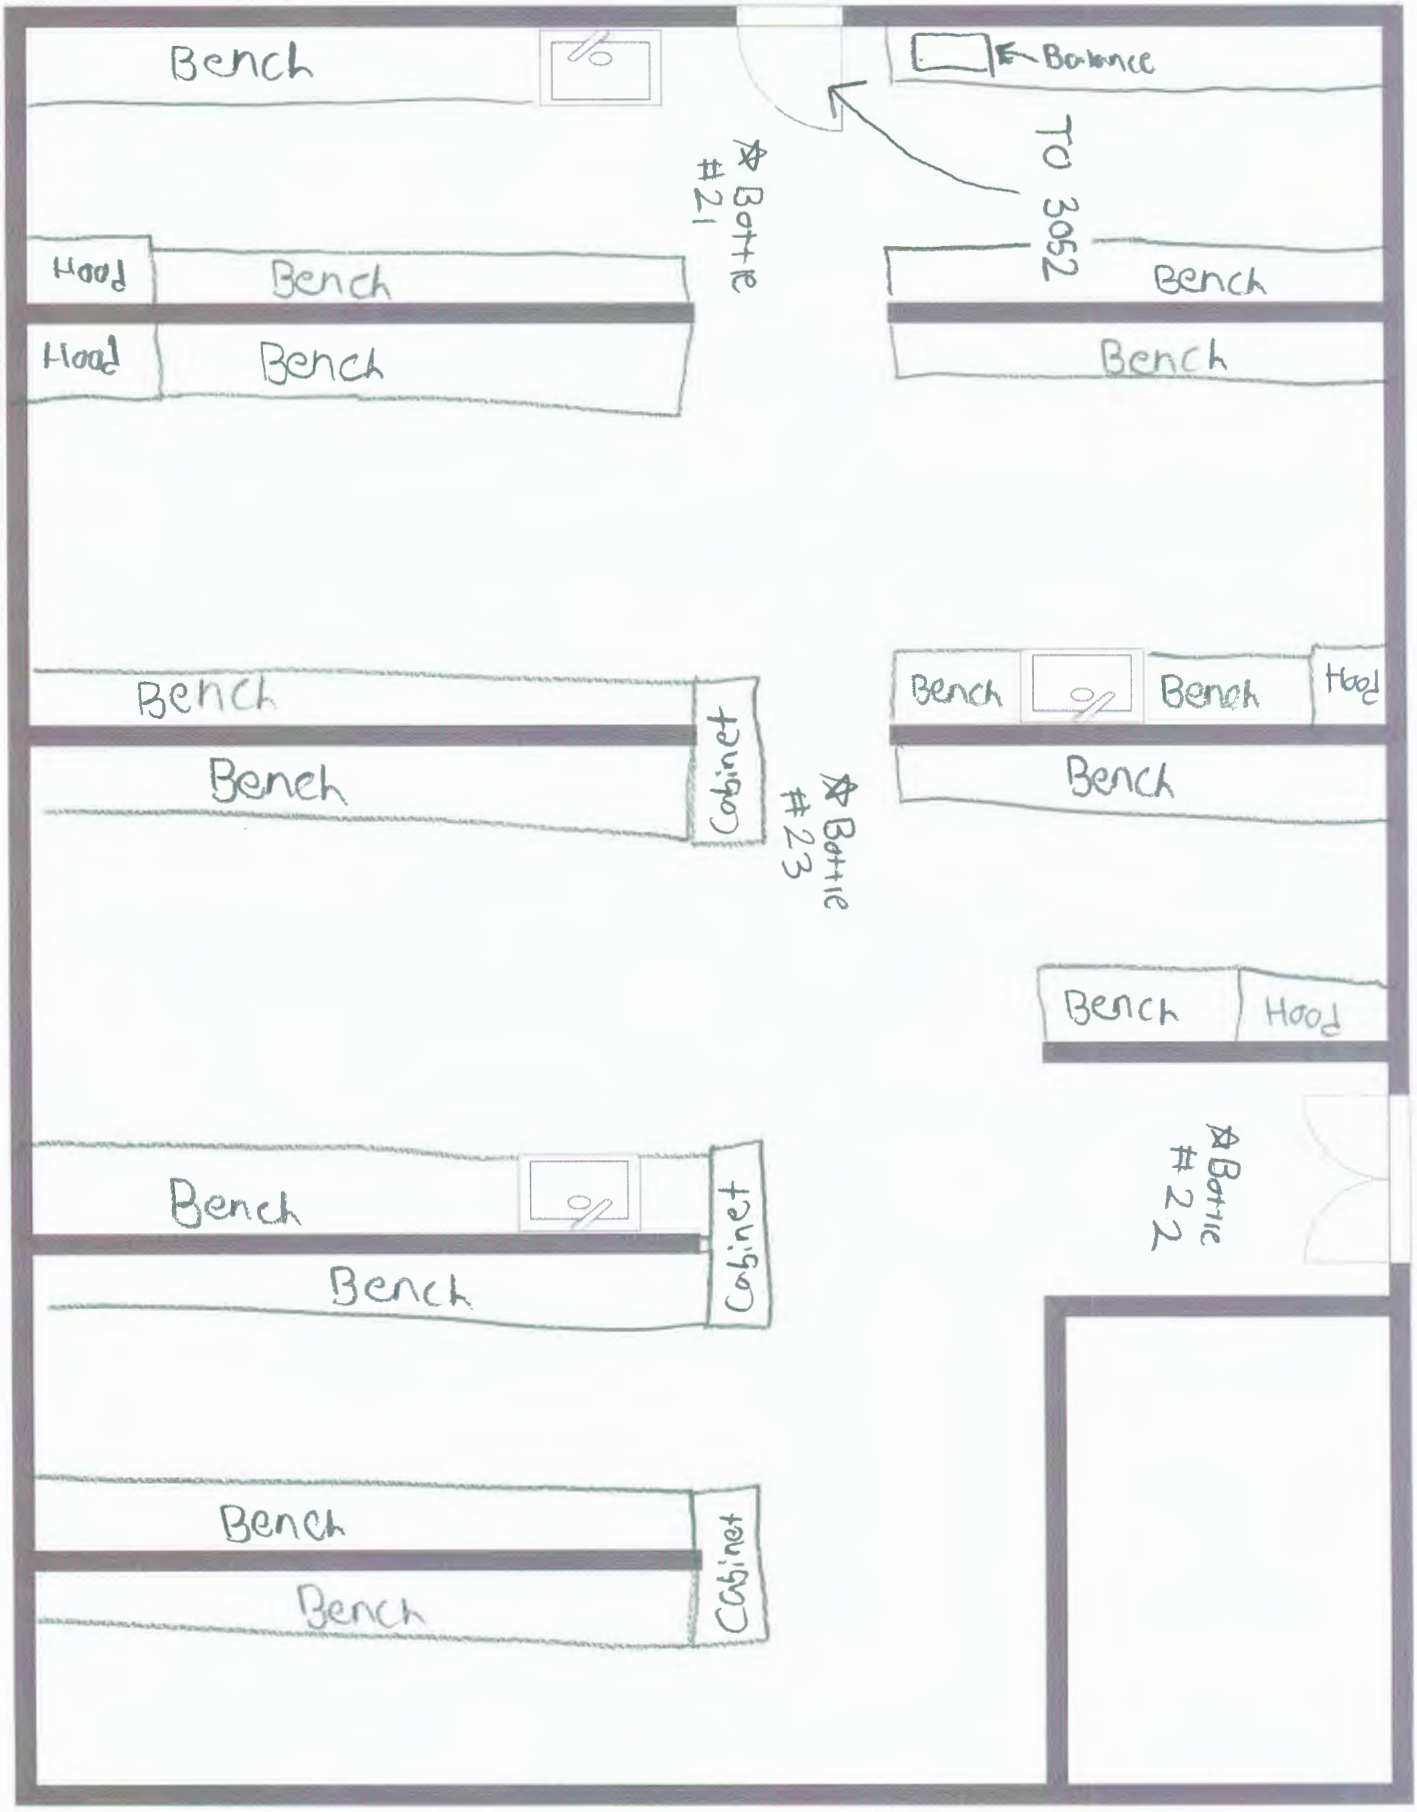

ESB 2062 Floor Plan

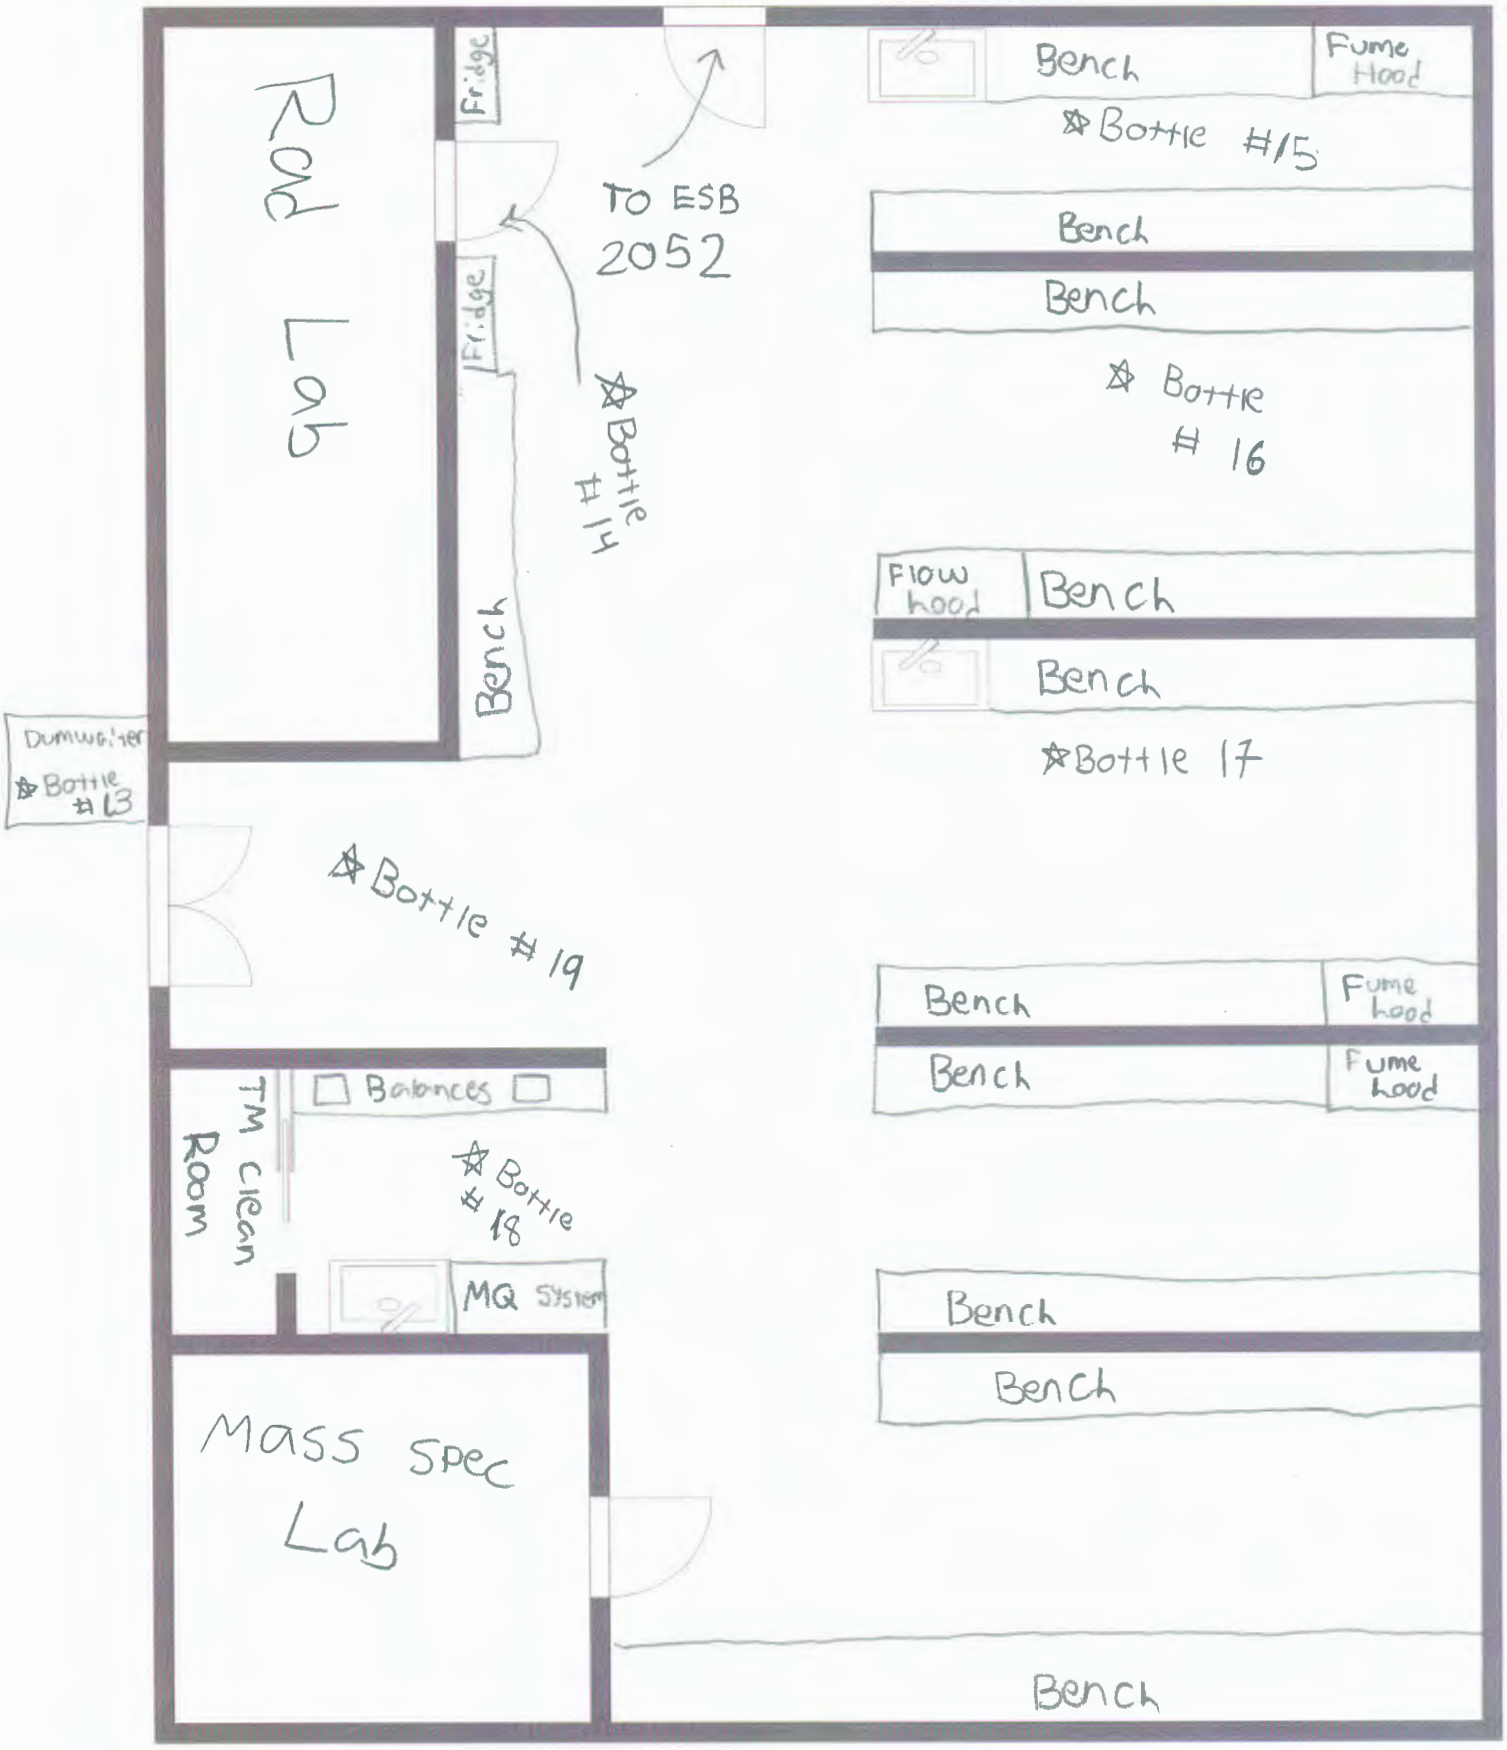

Closet in Groat Lab where I am moving my stuff (EOSM 313K)